



NOTE: Itemized order forms are available should that be your preference.

Level 1 Custom Products

Ride Custom AccuSoft Cushion and Custom Back with AccuSoft Foam Liner

Bundled Package Order Form

Client's First and Last Name*

Ride Custom AccuSoft Cushion (RCAC-S/RCAC-XS)

Shape provided via:

- RideWorks Scan
Java used as Evaluator Cushion

Ride Custom Back (RCB200)

Shape provided via:

- RideWorks Scan
Client measurements and finished product dimensions

NOTE: Only available with AccuSoft foam liner. See special instructions on page 11.

Account #

PO #

Date SO#

SN#

Date of shape capture:

*Internal management of personal information is HIPAA compliant.

General Information

Supplier

Ride Certified Practitioner Name

Address

City State Zip

Phone # Email

Ship to (if different from above)

NOTE: Ride Custom Systems must be fitted by a Ride Certified Provider and WILL NOT be drop shipped to end users.

Address

City State Zip

Phone # Email

Referral Source

Facility Name

Clinician Name

Phone # Email

Ride® Custom AccuSoft® Cushion and Custom Back Bundled Package

Client First and Last Name _____

Client Information

WARNING: Caution should be exercised when capturing shapes in Ride Simulators for people with osteoporosis, bone cancer, history of pathological fracture, osteogenesis imperfecta, or any brittle bone condition.

Sex: M F Diagnosis _____


Does client have:

- Current tissue injury? Location _____ Stage _____
- History of tissue injury? Location _____ Stage _____

Height _____ Weight _____

Client Measurements


- | | |
|---------------------------------|---|
| A. Trochanters _____" | G. Top of Iliac Crest L _____" R _____" |
| B. Leg length L _____" R _____" | H. Axilla height L _____" R _____" |
| C. Iliac Crest _____" | I. Top of shoulder L _____" R _____" |
| D. Mid-Thorax _____" | J. Knee to heel _____" |
| E. Axilla _____" | K. Top of head _____" |
| F. A-P Mid-Thorax _____" | L. A-P abdomen _____" |

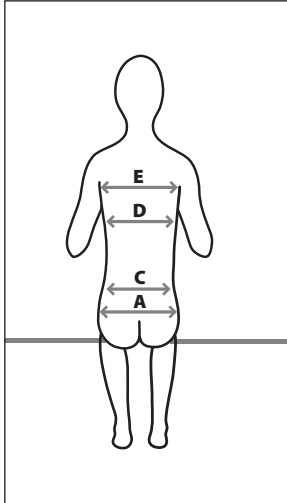

Mobility Base Specifications

Wheelchair Make _____ Model _____

Frame Width _____" Depth _____"

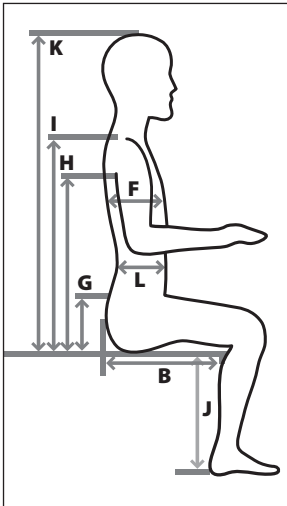


Ride Designs®
a branch of Aspen Seating, LLC



toll-free 866.781.1633
phone 303.781.1633
fax 303.781.1722

www.ridedesigns.com

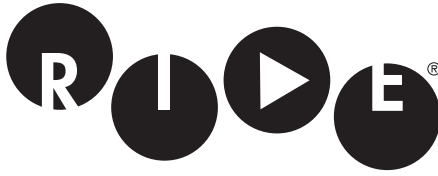

NOTE: Itemized order forms are available should that be your preference.

Ride® Custom AccuSoft® Cushion Bundled Package Order Form

Client First and Last Name _____

Prices effective January 8, 2024.

Item	Part Number	Mfr. Sugg. Retail Price*
<input type="checkbox"/> Ride Custom AccuSoft Cushion Soft - Bundled Medicare HCPCS Code E2609 Select outer covers:†	RCAC-S-B01	\$2931.00
<input type="checkbox"/> Outer breathable spacer fabric zip cover	RCAC-CBZ	
<input type="checkbox"/> Outer wipeable incontinence-resistant cover	RCAC-IC	
<input type="checkbox"/> Ride Custom AccuSoft Cushion Extra Soft - Bundled Medicare HCPCS Code E2609 Select outer covers:†	RCAC-XS-B01	\$2931.00
<input type="checkbox"/> Outer breathable spacer fabric zip cover	RCAC-CBZ	
<input type="checkbox"/> Outer wipeable incontinence-resistant cover	RCAC-IC	

NOTE: Every cushion comes standard with an inner moisture-resistant cover.

Shape Capture Process (please check one)

- Bead Bag
Indicate Shape Capture Base size used:
 Small (Blue) Medium (White)
 Large (Red) None
- Shape capture base is wedged up _____"
 Front Rear Left Side Right Side
 Build wedge into cushion per simulation RCAC-WS \$ 166.00
 Do not build wedge into cushion

- Scan of existing cushion (insert existing cushion measurements below)
Length L _____" R _____" Rear width _____" Front width _____"
Height at the following corners: Front L _____" Front R _____" Rear L _____" Rear R _____"
(Heights are not guaranteed if the cushion being scanned is a discontinued product.)

Is the existing cushion used on a sling seat? Yes No
(If yes, please note the new cushion will be made with a flat bottom. If the cushion being duplicated has a rounded bottom from use in the sling, this may result in height differences between the existing cushion and new cushion. Add the Bevel Cut option if the new cushion will be used on a sling seat.)

- Java® Cushion used to determine shape and dimensions (see instructions on page 5)

Resting Posture of Pelvis in Ride Shape Capture

- Neutral Posterior Anterior

* All prices are in U.S. dollars.

† Select one or both.

Ride® Custom AccuSoft® Cushion Bundled Package Order Form

Client First and Last Name _____

How to use a Java® Cushion to evaluate Custom AccuSoft Cushion specifications

Step 1

Sit client on an appropriately-sized Java Cushion.

Size used: Width _____" Length _____"

Step 2

Determine targeted cushion width in 1" increments.

Record targeted width in section 3 of the cushion order form.

Step 3

Determine targeted cushion length relative to the front of the Java Evaluator Cushion.

Measure from the front of the Java Cushion to establish cushion length.

Record targeted cushion length in section 4 of the cushion order form.

Step 4

Determine if additional lateral pelvic control is needed, adding Ride CAM Wedges to achieve this. Indicate where, and how many, Wedges were used.

The Ride Custom AccuSoft Cushion will be carved to match the contour created by Ride CAM Wedge placement.

No Wedges used

Wedges used on left side

0 1 2

Wedges used on right side

0 1 2

Step 5

Determine targeted sitting height and record in section 5 of the cushion order form.

Note: the height of the Java Cushion base and foam topper is as low as the Custom AccuSoft Cushion can be made.

Step 6

Determine whether wedges are needed under the Java Cushion during evaluation to achieve the desired position for correction or accommodation of pelvic/femoral asymmetries.

Record the usage of wedges here and record the targeted height in all four corners. Lateral height can be increased up to 2" from the top of the Java Evaluator Cushion.

Note: If more than 2" of additional lateral height is needed, please utilize Ride shape capture tools to capture and scan the shape.

Wedges used:

Front Back Left Side Right Side

Cushion height at corners:

Front Right _____" Front Left _____" Rear Right _____" Rear Left _____"

Step 7

Determine if additional medial and/or lateral thigh support is necessary in section 7 of the cushion order form.

Lateral height can be increased by up to 2" from the top of the Java Cushion, in 1" increments.

Note: If more than 2" of additional lateral height is needed, please utilize Ride shape capture tools to capture and scan the shape.

Step 8

Complete the remainder of the order form and email, along with photos of the client in the Java Evaluator Cushion, to: customerservice@ridedesigns.com.

**Proceed to Page 5
if a scanned shape
is being submitted.**

Ride® Custom AccuSoft® Cushion Bundled Package Order Form

Client First and Last Name _____

Photos and Scan

Using RideWorks? Use RideWorks app to:

- Photograph front and both sides of client during shape capture.
- Photograph captured shape.
- Scan captured shape.
- Take any and all additional photos that may help.

Not using RideWorks? Include:

- Photograph of front and side view of client during shape capture or evaluation in Java Cushion.
- Photograph of captured shape or of Java Cushion once evaluation is complete.

The Ride Custom AccuSoft Bundled Package includes all of the following options

Cushion Width (Actual cushion width will be 1/2" less than specified.)
 (Note: Cushion must not exceed wheelchair dimensions by more than 1" in any direction.)


Item	Part Number
Standard <input type="checkbox"/> 10" <input type="checkbox"/> 11" <input type="checkbox"/> 12" <input type="checkbox"/> 13" <input type="checkbox"/> 14" <input type="checkbox"/> 15" <input type="checkbox"/> 16" <input type="checkbox"/> 17" <input type="checkbox"/> 18" <input type="checkbox"/> 19" <input type="checkbox"/> 20"	RCAC-____ (width)
Extra large width <input type="checkbox"/> 21" <input type="checkbox"/> 22" <input type="checkbox"/> 23" <input type="checkbox"/> 24"	RCAC-W____ (width)
<input type="checkbox"/> Tapered width Back width _____" Front width _____"	RCAC-CWTW

**NOTE: Virtually any size cushion can be built.
Call for a quote.**

Cushion Length

(IMPORTANT: Specify cushion length relative to front of Shape Capture Base or Java Evaluator Cushion as shown.)
 Measure from front of Shape Capture Base or Java Evaluator Cushion to establish cushion length.
 (Note: Cushion must not exceed wheelchair dimensions by more than 1" in any direction.)

Item	Part Number
<input type="checkbox"/> Equal to Shape Capture Base length	RCAC-CLAC
Symmetrical Length	RCAC-CLSL
<input type="checkbox"/> Add _____" to Shape Capture Base length	
<input type="checkbox"/> Subtract _____" to Shape Capture Base length	
Asymmetrical Length	
LEFT	RCAC-CLALL
<input type="checkbox"/> Equal to Shape Capture Base length	
<input type="checkbox"/> Add _____" to Shape Capture Base length	
<input type="checkbox"/> Subtract _____" to Shape Capture Base length	
RIGHT	RCAC-CLALR
<input type="checkbox"/> Equal to Shape Capture Base length	
<input type="checkbox"/> Add _____" to Shape Capture Base length	
<input type="checkbox"/> Subtract _____" from Shape Capture Base length	

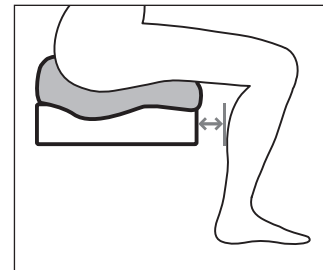


Missed this step? Indicate desired length of cushion on each side L _____" R _____"

<input type="checkbox"/> Undercut Front Edge 1"	RCAC-UC1
<input type="checkbox"/> Front rigging notches _____" W x _____" D x _____" H	RCAC-WCFR

Ride® Custom AccuSoft® Cushion Bundled Package Order Form
Client First and Last Name _____

Sitting Height

- Targeted final front cushion height (see diagrams at right) RCAC-SHTH No charge
 Height: L leg _____" R leg _____"
NOTE: This final height is not guaranteed. Results are dependent upon the accuracy of the captured shape. Height does not include cover thickness.

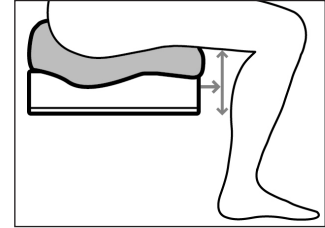

For targeted cushion height: at the projected cushion length, measure from the bottom of the shape capture base or Java Evaluator Cushion up to the underside of the leg with the feet properly positioned on the footplate(s).

Item	Part Number
<input type="checkbox"/> As captured	RCAC-SHAC
<input type="checkbox"/> Increase overall height _____"	RCAC-SHIH
<input type="checkbox"/> As low as possible	RCAC-SHDH

Cushion Contour

NOTE: The Custom AccuSoft Cushion is not a fully off-loading cushion. For highest level of skin protection, we recommend the Ride Custom 2 Cushion. (Requires Level 2 Certification).

- Ride contour RCAC-RC
 Cushion is manufactured with Ride's patented mechanism of support which reduces forces at high risk areas and provides slightly greater forces at low risk areas
NOTE: Ride contour is not available with Extra Soft Foam option.
- Full contact RCAC-FC
 Cushion manufactured as captured




Determine targeted front of cushion height (front view).

Thigh/Femoral Support

Item	Part Number
Medial Thigh Support If no selection is made, the medial thigh support will be manufactured as captured.	
<input type="checkbox"/> As captured	RCAC-MTAC
<input type="checkbox"/> Eliminate	RCAC-MTE
<input type="checkbox"/> Increase _____" (maximum 3" total height*)	RCAC-MTI
<input type="checkbox"/> Decrease _____"	RCAC-MTD
<input type="checkbox"/> Decrease as marked with line on Shape Capture Bag	RCAC-MTM

Lateral Thigh Support

LEFT	
<input type="checkbox"/> As captured	RCAC-LTAC
<input type="checkbox"/> Eliminate	RCAC-LTEL
<input type="checkbox"/> Increase _____" (maximum 3" total height*)	RCAC-LTIL
<input type="checkbox"/> Decrease _____"	RCAC-LTDL
<input type="checkbox"/> Decrease as marked with line on Shape Capture Bag	RCAC-LTML
RIGHT	
<input type="checkbox"/> As captured	RCAC-LTAC
<input type="checkbox"/> Eliminate	RCAC-LTER
<input type="checkbox"/> Increase _____" (maximum 3" total height*)	RCAC-LTIR
<input type="checkbox"/> Decrease _____"	RCAC-LTDR
<input type="checkbox"/> Decrease as marked with line on Shape Capture Bag	RCAC-LTMR

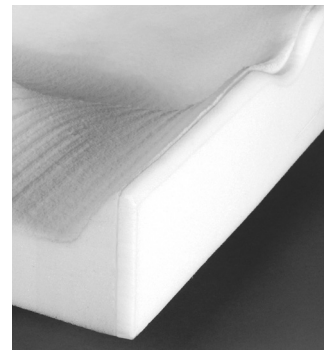

The Lateral Thigh Support Reinforcement option removes 1/2" of cushion foam from each lateral thigh support. Reinforcement material replaces the foam that was removed, without increasing the overall width of the cushion.

- Lateral Thigh Support Reinforcement RCAC-RL
 Boosts structural integrity while using forgiving materials that help reduce the risk of injury to skin and soft tissue. (Includes right and left sides.)

* As measured from lowest point of leg trough to top of medial or lateral thigh support

Ride® Custom AccuSoft® Cushion Bundled Package Order Form

Client First and Last Name _____

Cover Modifications

Item	Part Number
<input type="checkbox"/> For the outer breathable spacer fabric zip cover installed on cushion (if selected)	
<input type="checkbox"/> Spandex layer over spacer fabric	RCAC-SP
<input type="checkbox"/> Two-layer spacer fabric Soft Fit	RCAC-EM2

Custom AccuSoft Accessories

Item	Part Number
<input type="checkbox"/> 1" / 3cm Cushion Orientation Wedge (Note: These wedges are loose. To order a built-in wedge, please see pg 3.)	
<input type="checkbox"/> For 14" / 36cm cushion widths	RCAC-OW-1414
<input type="checkbox"/> For 15" / 38cm and 16" / 41cm cushion width	RCAC-OW-1616
<input type="checkbox"/> For 17" / 43cm and 18" / 46cm cushion widths	RCAC-OW-1816
<input type="checkbox"/> For 19" / 48cm and 20" / 51cm cushion widths	RCAC-OW-2016
Wedge to be used: (select one)	
<input type="checkbox"/> Outside cover	
<input type="checkbox"/> Inside cover	
If inside cover, thick edge of the wedge to be placed:	
<input type="checkbox"/> Back of cushion	
<input type="checkbox"/> Front of cushion	
<input type="checkbox"/> Left side of cushion	
<input type="checkbox"/> Right side of cushion	
<input type="checkbox"/> Ride CAM® Wedge Kit**	RCAC-WK

Cushion/Wheelchair Interface Modifications

Item	Part Number
<input type="checkbox"/> Bevel-Cut Modification for sling seat	RCAC-BC

Ride® Custom AccuSoft® Cushion Bundled Package Order Form

Client First and Last Name _____

Additional Options

Price not included in bundled package

Additional Cushion/Wheelchair Interface Options

Item	Part Number	Mfr. Sugg. Retail Price*
<input type="checkbox"/> Drop Seat Modification, 1" drop	RCAC-WC003	\$ 142.00
<input type="checkbox"/> Custom Mounting Platform (not compatible with bevel cut modification or drop seat modification) ABS platform with indexing tabs to ensure correct placement of cushion on seat	RCAC-CMP	\$ 450.00

Additional Cover Options

Item	Part Number	Mfr. Sugg. Retail Price*
<input type="checkbox"/> Additional breathable spacer fabric fabric zip cover	RCAC-CBZA ____ (width)	\$ 226.00
<input type="checkbox"/> Spandex layer over spacer fabric	RCAC-SP	\$ 86.00**
<input type="checkbox"/> Two-layer spacer fabric Soft Fit	RCAC-EM2	\$ 156.00**
<input type="checkbox"/> Additional outer incontinent-resistant cover Note: Only recommended for chronically incontinent clients. Does not replace inner, moisture-resistant cover.	RCAC-ICA	\$ 272.00
<input type="checkbox"/> Additional inner incontinent-resistant cover	RCAC-INICA	\$ 272.00

Growth

Item	Part Number	Mfr. Sugg. Retail Price*
<input type="checkbox"/> Growth Kit Provides for one growth adjustment, including one new inner cover and one new outer cover, during two year warranty period. Width and/or length, and/or height only. Changes in pelvic alignment and body shape can not be accommodated through growth adjustment. (This option requires shipping cushion to Ride Designs with RA.)	RCAC-DGK	\$ 279.00

We offer a 90 day fit and function guarantee and a two year warranty for all our custom products. Details can be found on our website at www.ridedesigns.com.

Total: _____

* All prices are in U.S. dollars.

** If these modifications were not selected with the included cushion cover, they will be provided at no charge with the additional cushion cover.

Special Instructions or Comments

NOTE: May affect price; call to request quote.

Pair the Ride Custom AccuSoft Cushion with a Ride Custom Back Support for optimal seating

Consider Ride Designs’ lightweight, thin-profile, and adjustable Custom Back support for the widest range of seating needs.

Breathable

Ultra-breathable 3D mesh liner material, along with a spacer fabric cover, help keep the sitter dry and comfortable in virtually any climate. (Requires Level 2 Certification)

Forgiving

An optional, soft open-cell polyurethane foam insert (AccuSoft Foam Liner) is available as an alternative to the ultra-breathable 3D mesh liner. This is the liner option available to Level 1 Certified Practitioners.

Protection and comfort

Supplementary padding and reliefs improve protection and comfort at sensitive areas.

Mounting options

Strong outer shell provides stability and surfaces for easy mounting of hardware and accessories.

Growable

Like the Ride Custom AccuSoft Cushion, the Back can be grown at a fraction of the cost of a new custom system.

More information at www.ridedesigns.com



Ride Custom Back paired with the Ride Custom AccuSoft Cushion.



Ride Designs®
a branch of Aspen Seating, LLC



toll-free 866.781.1633
phone 303.781.1633
fax 303.781.1722

www.ridedesigns.com
customerservice@ridedesigns.com



NOTE: Itemized order forms are available should that be your preference.

Ride® Custom Back with AccuSoft Foam Liner Bundled Package Order Form

Client First and Last Name _____

Prices effective January 8, 2024.

► Shape capture method

Using RideWorks® app?

Before scanning, on the clear, outer shape capture bag (using a black permanent marker), draw trim lines and marks to draw the back as it should be manufactured, including:

- Arrow pointing upward, indicating top of back
- Soft relief areas to protect bony prominences
- Depth and height of the lateral trunk supports



Before transferring client from shape capture bag, please complete the following...

PHOTOS of client in shape capture bag: Front view

Side view

- Included in RideWorks® client files
- Emailed to customerservice@ridedesigns.com, with client name and provider information
- Attached

DID YOU SEND PHOTOS?

Trim lines; establish and mark on clear, outer shape capture bag:

- Back height
- Lateral support depth and height
- Iliac crest height




► Using client measurements and final product dimensions? (No scan required. Only available with AccuSoft foam liner.)

Please see ordering instructions on page 11. Please skip to page 12 if ordering with a scan of a captured shape.

Ride® Custom Back Order Form
Client First and Last Name _____

Ordering with no scan - just client measurements and finished product dimensions. (Skip to pg 12 if submitting a scan.)

⚠ Important: Clients who present with significant postural asymmetries and require substantial support to maintain optimal posture will experience the best outcome with a Ride Custom Back made from a captured shape that is scanned and submitted to Ride.

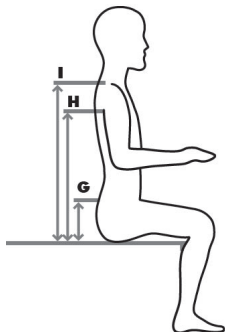


Step 1 - Client Measurements


Make sure the following client measurements are provided, either on page 2, or here:

- G. Top of Iliac Crest L _____ " R _____ "
- H. Axilla Height L _____ " R _____ "
- I. Top of Shoulder L _____ " R _____ "

Step 2 - Desired finished back height _____ "




Step 3 - Desired finished lateral height from seat to top of lateral. (For full-height lateral pads, this number should equal "tall" lateral pad measurement in step 4.)




- 3a. Client's left side top of lateral _____ "
- 3b. Client's right side top of lateral _____ "

Step 4 - Desired finished lateral pad dimensions (Min. 3" tall.) (Maximum lateral depth, 7". If lateral depth greater than 7" is needed, please capture a shape, scan the shape and submit the scan via the RideWorks app.)



- 4a. Client left lateral pad _____ " tall x _____ " deep
- 4b. Client right lateral pad _____ " tall x _____ " deep

Step 5 - Desired finished outside back width _____ " (Foam liner will result in inside width being approximately 2" narrower than outside width).

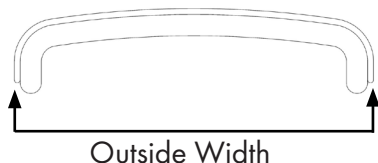

Ride® Custom Back with AccuSoft Foam Liner Bundled Package Order Form
Client First and Last Name _____

Item	Part Number	Mfr. Sugg. Retail Price*
------	-------------	--------------------------


- | | | |
|---|---------------|------------|
| <input type="checkbox"/> Ride Custom Back - Bundled
Medicare HCPCS Code E2617
Custom contoured back shell;
AccuSoft® foam liner; and choice of spacer fabric cover
or wipeable, incontinence-proof cover.
Note: 3D mesh liner is only available to Level 2 Certified Practitioners. | RCB200 Bundle | \$ 3847.00 |
|---|---------------|------------|

The RCB200 Bundled Package includes all of the following options

Ride Custom Back Width

Item	Part Number
------	-------------

Find the widest spot on client's body in between axilla and trochanters and provide the measurement _____ "

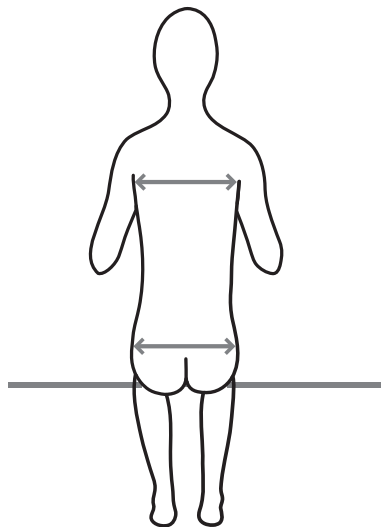

- Widest spot is < 20" RCB2-200R
- Widest spot is 21" - 24" RCB2-200W

Pricing for widths greater than 24" will be individually determined and quoted.

Minimum back height requirements for headrest accessory use		
Headrest Type	with Single Hardware	with Double Hardware
None	7"/0.178m	12"/0.330m
Universal Headrest Mounting Plate	11.5"/0.292m	18"/0.457m
Integrated Headrest/Accessories Mount	9.5"/0.241m	15.5"/0.394m

NOTE: Measure back height from top trimline to bottom trimline.

Ride Custom Back Hardware and Mounting - First Set

Item	Part Number
------	-------------

Ride FlexLoc® Hardware

NOTE: Sections a, b, and c **MUST** have a selection.

a. Select Size:

NOTE: Order the hardware size that matches the distance between mounting locations, not necessarily the wheelchair width. Mounting FlexLoc to Permobil or Quantum requires small FlexLoc mounting hardware with FlexLoc adapter plates from Ride Designs, Direct Backrest Frame from Permobil or aftermarket back interface from Quantum.

*WARNING! Two (2) sets of FlexLoc hardware are required if the client presents with any of the following:

- Weight exceeds 250 pounds
- Overall back height measurement (as measured to trim lines on cast) is greater than or equal to 28"
- Severe extensor tone, spasticity, etc.

First Set of Hardware (First set is included in the bundled price. If two sets of hardware are needed, select the second set on page 14.)

- | | |
|--|-------------|
| <input type="checkbox"/> Small, mounting distance 10 - 14" | RCB2-FL-MS |
| <input type="checkbox"/> Medium, mounting distance 15 - 18" | RCB2-FL-MM |
| <input type="checkbox"/> Large, mounting distance 19 - 21" | RCB2-FL-ML |
| <input type="checkbox"/> X-Large, mounting distance 22 - 24" | RCB2-FL-MX |
| <input type="checkbox"/> Omit hardware | RCB2-200R-0 |

b. Select Mounting for first set of hardware:

Clamp Mount for round back canes RCB2-FL-MCI

Quickie Sedeo Pro Interface Bracket RCB2-QSIB

Mounts RCB200 to Quickie Sedeo Pro Power Seating System.

- Not compatible with Quickie Sedeo Pro Advanced seating system.
- Not compatible with tilt-only Sedeo Pro seating system. *Call for mounting options for tilt-only.*
- Available as a single-mount option. *Call for options if double hardware is needed on a Sedeo Pro seating system.*
- Order small FlexLoc hardware for use with this option.
- This option replaces cane clamps.

Order small FlexLoc hardware for use with this option. This option replaces cane clamps.

FlexLoc Adapter Plate RCB2-FL-MCI-P1

For mounting to wheelchairs without round back canes, e.g. Permobil 3G, Invacare Tilt and Recline, or general surface mounting to existing back pans. This option replaces cane clamps.

c. Select Attachment for first set of hardware:


Fixed, non-removeable RCB2-FL-FMI

Quick Release Option RCB2-FL-QR

NOTE: The Ride FlexLoc Mount can be interfaced with most any wheelchair configuration. Contact Ride Designs for a solution to your mounting challenge.



Ride FlexLoc Hardware

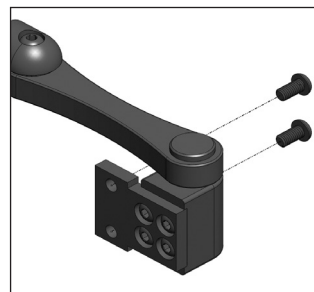

Adapter Plate



Quick Release Option

Ride® Custom Back with AccuSoft Foam Liner Bundled Package Order Form
Client First and Last Name _____

Foam Liner

Item	Part Number
Note: 3D Mesh liner is only available to Level 2 Certified Practitioners	
<input type="checkbox"/> AccuSoft foam liner (increases each lateral support thickness by ½" and may result in compromise of postural correction)	RCB2-FS
Select one cover:	
<input type="checkbox"/> Spacer fabric cover	RCB2-SFC
<input type="checkbox"/> Wipeable, incontinence-proof cover	RCB2-IC



AccuSoft foam liner


Supplementary Padding, Reliefs, Dimensions

Item	Part Number
Extended depth lateral thoracic support	
<input type="checkbox"/> Extend LEFT lateral thoracic support _____" forward of reference line.	RCB2-EDLTS-L
<input type="checkbox"/> Extend RIGHT lateral thoracic support _____" forward of reference line.	RCB2-EDLTS-R
— Mark reference line(s) on clear, outer shape capture bag, or on cast if not using RideWorks.	
<input type="checkbox"/> Enhanced relief	RCB2-ERFP
Typically used for improved protection and comfort at specific skeletal prominences such as rib humps and spinous processes.	
— Draw desired location(s) and shape of relief on clear, outer shape capture bag, or on cast if not using RideWorks.	
Extended height lateral thoracic support	
<input type="checkbox"/> Increase LEFT lateral thoracic support _____" above reference line.	RCB2-EHLTS-L
<input type="checkbox"/> Increase RIGHT lateral thoracic support _____" above reference line.	RCB2-EHLTS-R
Extended back height	
<input type="checkbox"/> Extend back height _____" above reference line.	RCB2-EBH
— Mark reference line(s) on clear, outer shape capture bag, or on cast if not using RideWorks.	


Ride® Custom Back with AccuSoft Foam Bundled Package Order Form
Client First and Last Name _____

Accessories

Item	Part Number
<input type="checkbox"/> Universal headrest mounting plate, installed Note: Will be installed midline, top of back, unless otherwise marked on clear, outer shape capture bag, or on cast if not using RideWorks.	RCB2-UHMP
<input type="checkbox"/> Integrated headrest/accessories mount Note: May be mounted to FlexLoc vertical track if back height is not sufficient for an integrated mount.	RCB2-AM
<input type="checkbox"/> Shoulder harness guides, pair, loose	RCB2-SHG
<input type="checkbox"/> Shoulder harness guides, pair, installed Note: Mark location on clear, outer shape capture bag, or on cast if not using RideWorks.	RCB2-SHGI

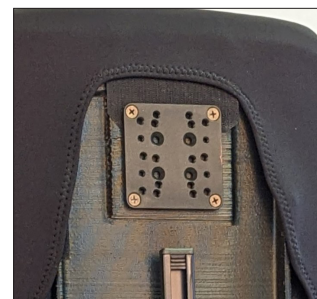

Universal Headrest Mounting Plate.

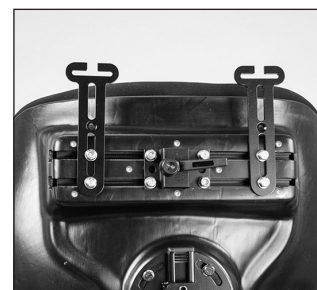

Integrated Headrest/Accessories Mount with Shoulder Harness Guides and headrest mount installed.

Additional Options

Price not included in bundled package

Additional Hardware and Mounting Options

Item	Part Number	Mfr. Sugg. Retail Price*
------	-------------	--------------------------

Ride FlexLoc® Hardware - Second Set

a. Select Size:

NOTE: Order the hardware size that matches the distance between mounting locations, not necessarily the wheelchair width. Mounting FlexLoc to Permobil or Quantum requires small FlexLoc mounting hardware with FlexLoc adapter plates from Ride Designs, Direct Backrest Frame from Permobil or aftermarket back interface from Quantum.

*WARNING! Two (2) sets of FlexLoc hardware are required if the client presents with any of the following:

- Weight exceeds 250 pounds
- Overall back height measurement (as measured to trim lines on cast) is greater than or equal to 28"
- Severe extensor tone, spasticity, etc.

<input type="checkbox"/> Second Set of FlexLoc Hardware		
<input type="checkbox"/> Small, mounting distance 10 - 14"	RCB2-FL-MS	\$ 590.00
<input type="checkbox"/> Medium, mounting distance 15 - 18"	RCB2-FL-MM	\$ 590.00
<input type="checkbox"/> Large, mounting distance 19 - 21"	RCB2-FL-ML	\$ 590.00
<input type="checkbox"/> X-Large, mounting distance 22 - 24"	RCB2-FL-MX	\$ 590.00

b. Select Mounting for second set of hardware:

<input type="checkbox"/> Clamp Mount for round back canes	RCB2-FL-MCI	\$ 0.00
<input type="checkbox"/> Additional Mounting Clamps (pair) NOTE: If ordering Double FlexLoc mounting hardware, two sets of mounting clamps are included.	RCB2-FL-MC	\$ 238.00
<input type="checkbox"/> FlexLoc Adapter Plate For mounting to wheelchairs without round back canes, e.g. Permobil 3G, Invacare Tilt and Recline, or general surface mounting to existing back pans. This option replaces Cane Clamps.	RCB2-FL-MCI-PT	\$ 0.00

c. Select Attachment type for second set of hardware:

<input type="checkbox"/> Fixed, non-removable	RCB2-FL-FMI	\$ 0.00
<input type="checkbox"/> Quick Release Option	RCB2-FL-QR	\$ 97.00

PHOTOS??
JUST CHECKING.

* All prices are in U.S. dollars.

Additional Supplementary Padding, Reliefs, Dimensions

Item	Part Number	Mfr. Sugg. Retail Price*
Axillary support pad Typically used for distribution of corrective forces near the axilla on concave side of scoliosis.		
<input type="checkbox"/> Left	RCB2-ASP-L	\$ 207.00
<input type="checkbox"/> Right	RCB2-ASP-R	\$ 207.00
<input type="checkbox"/> Vertical back reinforcement	RCB2-RBS	\$ 332.00
<input type="checkbox"/> Reinforced lateral thoracic supports	RCB2-RLTS	\$ 450.00

Note: No longer required for lateral supports more than 6" deep. It is not possible to adjust lateral width on the RCB200 by bending the lateral reinforcement. Modifications to lateral support width must be made by heating the RCB200 shell.

Additional accessories

Item	Part Number	Mfr. Sugg. Retail Price*
Privacy flap Covers gap between cushion and back support.		
Size		
<input type="checkbox"/> Small — fits wheelchair widths less than 14"	RCB2-PFS	\$ 155.00
<input type="checkbox"/> Medium — fits wheelchair widths 15 - 17"	RCB2-PFM	\$ 155.00
<input type="checkbox"/> Large — fits wheelchair widths 18" and larger	RCB2-PFL	\$ 155.00



Privacy flap covers the space between the cushion and back support.

Abdominal support panel

Instructions:

1. Before removing client from back shape capture bag, mark height of each ASIS on clear, outer bag.
2. Measure up from this mark to establish desired height of abdominal panel needed.
3. Ride Designs will install the abdominal panel for you to meet these specifications.

Size

<input type="checkbox"/> Small — height 4" (two straps) Measurement around abdomen _____"	RCB2-AP-4	\$ 408.00
<input type="checkbox"/> Medium — height 6" (three straps) Measurement around abdomen _____"	RCB2-AP-6	\$ 408.00
<input type="checkbox"/> Large — height 8" (three straps) Measurement around abdomen _____"	RCB2-AP-8	\$ 408.00



Abdominal Support Panel.

Ride® Custom Back with Accusoft Foam Liner Bundled Package Order Form
Client First and Last Name _____

Additional Covers

Item	Part Number	Mfr. Sugg. Retail Price*
<input type="checkbox"/> Additional breathable cover	RCB2-SFCA	\$ 384.00
<input type="checkbox"/> Additional wipeable, incontinence-proof cover	RCB2-ICA	\$ 384.00

Growth

Item	Part Number	Mfr. Sugg. Retail Price*
<input type="checkbox"/> Growth Kit Provides for one growth adjustment, including a new cover, during two year warranty period. Width and/or height only. Changes in spinal alignment and body shape can not be accommodated through growth adjustment.	RCB2-DGK	\$ 512.00

Total: _____

Special Instructions or Comments

NOTE: May affect price; call to request quote.

We offer a 90 day fit and function guarantee and a two year warranty for all our custom products. Details can be found on our website at www.ridedesigns.com.

PHOTOS??
 THEY MUST BE
 HERE SOMEWHERE.



Ride Designs®
 a branch of Aspen Seating, LLC



toll-free 866.781.1633
 phone 303.781.1633
 fax 303.781.1722

www.ridedesigns.com
customerservice@ridedesigns.com