



Ride® Custom Order Form for Level 1 Certified Practitioners
Ride Custom AccuSoft® Cushion and Custom Back w/AccuSoft Foam Liner

Client's First and Last Name\* \_\_\_\_\_

[ ] Ride® Custom AccuSoft® Cushion (RCAC-S/RCAC-XS)

Shape provided via:

- [ ] RideWorks® Scan
[ ] Java® Cushion used as Evaluator tool
[ ] Other

[ ] Ride Custom Back with AccuSoft foam liner (RCB200)

Shape provided via:

- [ ] RideWorks Scan
[ ] Client Measurements and Finished Product Dimensions

NOTE: Only available with AccuSoft foam liner. See special instructions on page 10.

Account # \_\_\_\_\_
PO # \_\_\_\_\_
Date \_\_\_\_\_ SO# \_\_\_\_\_
SN# \_\_\_\_\_

Date of shape capture: \_\_\_\_\_

\*Internal management of personal information is HIPAA compliant.

General Information

Supplier \_\_\_\_\_

Ride Level 1 Certified Practitioner Name \_\_\_\_\_

Address \_\_\_\_\_

City \_\_\_\_\_ State \_\_\_\_\_ Zip \_\_\_\_\_

Phone # \_\_\_\_\_ Email \_\_\_\_\_

Ship to (if different from above)

NOTE: Ride Custom Systems must be fitted by a Ride Certified Provider and WILL NOT be drop shipped to end users.

Address \_\_\_\_\_

City \_\_\_\_\_ State \_\_\_\_\_ Zip \_\_\_\_\_

Phone # \_\_\_\_\_ Email \_\_\_\_\_

Referral Source

Facility Name \_\_\_\_\_

Clinician Name \_\_\_\_\_

Phone # \_\_\_\_\_ Email \_\_\_\_\_

**Ride® Custom AccuSoft® Cushion and Custom Back with AccuSoft Foam Liner**

Client First and Last Name \_\_\_\_\_

**Client Information**

WARNING: Caution should be exercised when capturing shapes in Ride Simulators for people with osteoporosis, bone cancer, history of pathological fracture, osteogenesis imperfecta, or any brittle bone condition.

Sex:  M  F Diagnosis \_\_\_\_\_

Does client have:


Current tissue injury? Location \_\_\_\_\_ Stage \_\_\_\_\_

History of tissue injury? Location \_\_\_\_\_ Stage \_\_\_\_\_

Height \_\_\_\_\_ Weight \_\_\_\_\_

**Client Measurements**


- |                                 |   |
|---------------------------------|---|
| A. Trochanters _____"           | G. Top of Iliac Crest L _____" R _____" |
| B. Leg length L _____" R _____" | H. Axilla height L _____" R _____"      |
| C. Iliac Crest _____"           | I. Top of shoulder L _____" R _____"    |
| D. Mid-Thorax _____"            | J. Knee to heel _____"                  |
| E. Axilla _____"                | K. Top of head _____"                   |
| F. A-P Mid-Thorax _____"        | L. A-P abdomen _____"                   |

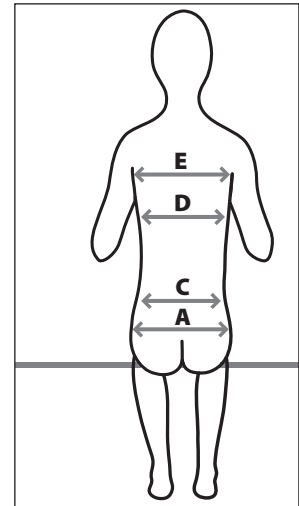

**Mobility Base Specifications**

Wheelchair Make \_\_\_\_\_ Model \_\_\_\_\_

Frame Width \_\_\_\_\_" Depth \_\_\_\_\_"

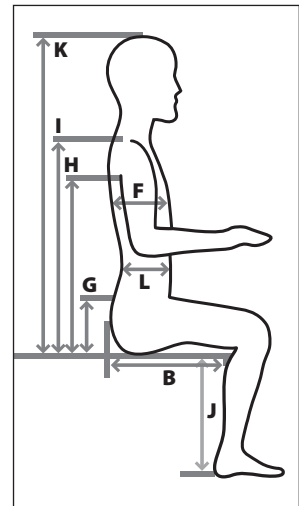



# Ride® Custom AccuSoft® Cushion Order Form

Client First and Last Name \_\_\_\_\_

Prices effective January 8, 2024.

Item	Part Number	Mfr. Sugg. Retail Price*
<input type="checkbox"/> Ride Custom AccuSoft Cushion - Soft Medicare HCPCS Code E2609 Select one outer cover:†	RCAC-S	\$2175.00
<input type="checkbox"/> Outer breathable spacer fabric zip cover	RCAC-CBZ	
OR		
<input type="checkbox"/> Outer wipeable incontinence-resistant cover	RCAC-IC	
<input type="checkbox"/> Ride Custom AccuSoft Cushion - Extra Soft Medicare HCPCS Code E2609 Select one outer cover: †	RCAC-XS	\$2175.00
<input type="checkbox"/> Outer breathable spacer fabric zip cover	RCAC-CBZ	
OR		
<input type="checkbox"/> Outer wipeable incontinence-resistant cover	RCAC-IC	

**NOTE: Every cushion comes standard with an inner moisture-resistant cover.**

## Shape Capture Process (please check one)

- Bead Bag  
Indicate Shape Capture Base size used:
  - Small (Blue)     Medium (White)
  - Large (Red)     None
  
- Shape Capture Base is Wedged Up \_\_\_\_\_"
  - Front     Rear
  - Left Side     Right Side
  - Build wedge into cushion per simulation.                      RCAC-WS                      \$ 166.00
  - Do not build wedge into cushion.
  
- Scan of existing cushion (insert existing cushion measurements below)
 

Length L \_\_\_\_\_" R \_\_\_\_\_"    Rear width \_\_\_\_\_" Front width \_\_\_\_\_"

Height at the following corners: Front L \_\_\_\_\_" Front R \_\_\_\_\_" Rear L \_\_\_\_\_" Rear R \_\_\_\_\_"

(Heights are not guaranteed if the cushion being scanned is a discontinued product.)

Is the existing cushion used on a sling seat?     Yes     No

(If yes, please note the new cushion will be made with a flat bottom. If the cushion being duplicated has a rounded bottom from use in the sling, this may result in height differences between the existing cushion and new cushion. Add the Bevel Cut option if the new cushion will be used on a sling seat.)
  
- Java® Cushion used to determine shape and dimensions (see instructions on page 5)

## Resting Posture of Pelvis in Ride Shape Capture

- Neutral     Posterior     Anterior

\* All prices are in U.S. dollars.

† Additional covers available in Section 8.

# Ride® Custom AccuSoft® Cushion Order Form

Client First and Last Name \_\_\_\_\_

## 1. Photos and Scan

**Using RideWorks?** Use RideWorks app to:

- Photograph front and both sides of client during shape capture.
- Photograph captured shape.
- Scan captured shape.
- Take any and all additional photos that may help.

**Not using RideWorks?** Include:

- Photograph of front and side view of client during shape capture or evaluation in Java Cushion.
- Photograph of captured shape or of Java Cushion once evaluation is complete.

## 2. Cushion/Wheelchair Interface (Flat bottom for solid seat is standard.)

Item	Part Number	Mfr. Sugg. Retail Price*
<input type="checkbox"/> Bevel-Cut Modification for sling seat	RCAC-BC	\$ 142.00
<input type="checkbox"/> Drop Seat Modification, 1" drop	RCAC-WC003	\$ 142.00
<input type="checkbox"/> Custom Mounting Platform ABS platform with indexing tabs to ensure correct placement of cushion on seat (not compatible with bevel cut or drop seat modification)	RCAC-CMP	\$ 450.00

## 3. Cushion Width (Actual cushion width will be 1/2" less than specified.)

(Note: Cushion must not exceed wheelchair dimensions by more than 1" in any direction.)

Item	Part Number	Mfr. Sugg. Retail Price*
Standard <input type="checkbox"/> 10" <input type="checkbox"/> 11" <input type="checkbox"/> 12" <input type="checkbox"/> 13" <input type="checkbox"/> 14" <input type="checkbox"/> 15" <input type="checkbox"/> 16" <input type="checkbox"/> 17" <input type="checkbox"/> 18" <input type="checkbox"/> 19" <input type="checkbox"/> 20"	RCAC-____ (width)	No charge
Extra large width <input type="checkbox"/> 21" <input type="checkbox"/> 22" <input type="checkbox"/> 23" <input type="checkbox"/> 24"	(width) RCAC-W____	\$ 147.00
<input type="checkbox"/> Tapered width Back width _____" Front width _____"	RCAC-CWTW	\$ 147.00

**NOTE: Virtually any size cushion can be built.  
Call for a quote.**


## 4. Cushion Length

(IMPORTANT: Specify cushion length relative to front of Shape Capture Base or Java Evaluator Cushion as shown.)

Measure from front of Shape Capture Base or Java Evaluator Cushion to establish cushion length.

(Note: Cushion must not exceed wheelchair dimensions by more than 1" in any direction.)

Item	Part Number	Mfr. Sugg. Retail Price*
<input type="checkbox"/> Equal to Shape Capture Base length	RCAC-CLAC	Standard
Symmetrical Length <input type="checkbox"/> Add _____" to Shape Capture Base length <input type="checkbox"/> Subtract _____" to Shape Capture Base length	RCAC-CLSL	No charge
Asymmetrical Length		\$ 142.00
LEFT	RCAC-CLALL	
<input type="checkbox"/> Equal to Shape Capture Base length <input type="checkbox"/> Add _____" to Shape Capture Base length <input type="checkbox"/> Subtract _____" to Shape Capture Base length		
RIGHT	RCAC-CLALR	
<input type="checkbox"/> Equal to Shape Capture Base length <input type="checkbox"/> Add _____" to Shape Capture Base length <input type="checkbox"/> Subtract _____" from Shape Capture Base length		

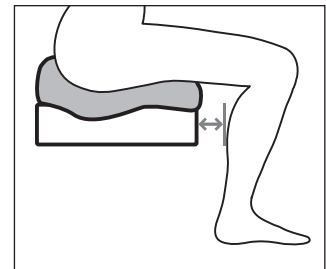

Missed this step? Indicate desired length  
of cushion on each side L \_\_\_\_\_" R \_\_\_\_\_"

# Ride® Custom AccuSoft™ Cushion Order Form

Client First and Last Name \_\_\_\_\_

---

## How to use a Java® Cushion to evaluate Custom AccuSoft Cushion specifications

### Step 1

Sit client on an appropriately-sized Java Cushion.

Size used: Width \_\_\_\_\_" Length \_\_\_\_\_"

Proceed to Page 6  
if a scanned shape  
is being submitted.

### Step 2

Determine targeted cushion width in 1" increments.

Record targeted width in section 3 of the cushion order form.

### Step 3

Determine targeted cushion length relative to the front of the Java Evaluator Cushion.

Measure from the front of the Java Cushion to establish cushion length.

Record targeted cushion length in section 4 of the cushion order form.

### Step 4

Determine if additional lateral pelvic control is needed, inserting Ride CAM Wedges into the slots in the rear of the Java Cushion base to achieve this. Indicate where, and how many, Wedges were used.

The Ride Custom AccuSoft Cushion will be carved to match the contour created by Ride CAM Wedge placement.

No Wedges used

Wedges used on left side

0  1  2

Wedges used on right side

0  1  2

### Step 5

Determine targeted sitting height and record in section 5 of the cushion order form.

Note: the height of the Java Cushion base and foam topper is as low as the Custom AccuSoft Cushion can be made.

### Step 6

Determine whether wedges are needed under the Java Cushion during evaluation to achieve the desired position for correction or accommodation of pelvic/femoral asymmetries.

Record the usage of wedges here and record the targeted height in all four corners. Lateral height can be increased up to 2" from the top of the Java Evaluator Cushion.

Note: If more than 2" of additional lateral height is needed, please utilize Ride shape capture tools to capture and scan the shape.

Wedges used:

Front  Back  Left Side  Right Side

Cushion height at corners:

Front Right \_\_\_\_\_" Front Left \_\_\_\_\_" Rear Right \_\_\_\_\_" Rear Left \_\_\_\_\_"

### Step 7

Determine if additional medial and/or lateral thigh support is necessary in section 7 of the cushion order form.

Lateral height can be increased by up to 2" from the top of the Java Cushion, in 1" increments.

Note: If more than 2" of additional lateral height is needed, please utilize Ride shape capture tools to capture and scan the shape.

### Step 8

Complete the remainder of the order form and email, along with photos of the client in the Java Evaluator Cushion, to: [customerservice@ridedesigns.com](mailto:customerservice@ridedesigns.com).

**Page 5**


Continue on page 6

# Ride® Custom AccuSoft® Cushion Order Form

Client First and Last Name \_\_\_\_\_

## 5. Sitting Height


Item	Part Number	Mfr. Sugg. Retail Price*
<input type="checkbox"/> Targeted final front cushion height (see diagrams at right) Height: L leg _____" R leg _____" NOTE: This final height is not guaranteed. Results are dependent upon the accuracy of the captured shape. Height does not include cover thickness.	RCAC-SHTH	No charge
<input type="checkbox"/> As captured	RCAC-SHAC	Standard
<input type="checkbox"/> Increase overall height _____"	RCAC-SHIH	\$ 166.00
<input type="checkbox"/> As low as possible	RCAC-SHDH	\$ 166.00

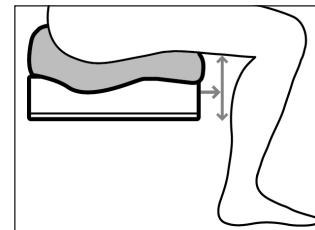

For targeted cushion height: at the projected cushion length, measure from the bottom of the shape capture base or Java Evaluator Cushion up to the underside of the leg with the feet properly positioned on the footplate(s).

## 6. Cushion Contour

Item	Part Number	Mfr. Sugg. Retail Price*
<b>**NOTE: The Custom AccuSoft Cushion is not a fully off-loading cushion. For highest level of skin protection, we recommend the Ride Custom 2 Cushion.</b>		
<input type="checkbox"/> Ride contour** Cushion is manufactured with Ride's patented mechanism of support which reduces forces at high risk areas and provides slightly greater forces at low risk areas. NOTE: Ride contour is not available with Extra Soft Foam option.	RCAC-RC	No charge
<input type="checkbox"/> Reticulated foam well insert kit For gentle support to bony prominences and to maintain a high level of microclimate management. ⚠️ONE SIZE: Must be trimmed in field to fit.	RCAC-WI	\$52.00
<input type="checkbox"/> Full contact** Cushion manufactured as captured	RCAC-FC	No charge

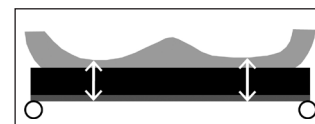

Determine targeted front of cushion height (front view).

## 7. Thigh/Femoral Support

Item	Part Number	Mfr. Sugg. Retail Price*
<b>Medial Thigh Support</b> If no selection is made, the medial thigh support will be manufactured as captured.		
<input type="checkbox"/> As captured	RCAC-MTAC	Standard
<input type="checkbox"/> Eliminate	RCAC-MTE	No charge
<input type="checkbox"/> Increase _____" (maximum 3" total height from bottom of leg trough)	RCAC-MTI	\$ 126.00
<input type="checkbox"/> Decrease _____"	RCAC-MTD	No charge
<input type="checkbox"/> Decrease as marked with line on Shape Capture Bag	RCAC-MTM	No charge

### Lateral Thigh Support


LEFT

<input type="checkbox"/> As captured	RCAC-LTAC	Standard
<input type="checkbox"/> Eliminate	RCAC-LTEL	No charge
<input type="checkbox"/> Increase _____" (maximum 3" total height from bottom of leg trough)	RCAC-LTIL	\$ 126.00
<input type="checkbox"/> Decrease _____"	RCAC-LTDL	No charge
<input type="checkbox"/> Decrease as marked with line on Shape Capture Bag	RCAC-LTML	No charge

RIGHT

<input type="checkbox"/> As captured	RCAC-LTAC	Standard
<input type="checkbox"/> Eliminate	RCAC-LTER	No charge
<input type="checkbox"/> Increase _____" (maximum 3" total height from bottom of leg trough)	RCAC-LTIR	\$ 126.00
<input type="checkbox"/> Decrease _____"	RCAC-LTDR	No charge
<input type="checkbox"/> Decrease as marked with line on Shape Capture Bag	RCAC-LTMR	No charge

<input type="checkbox"/> Lateral Thigh Support Reinforcement Boosts structural integrity while using forgiving materials that help reduce the risk of injury to skin and soft tissue. (Includes right and left sides.)	RCAC-RL	\$ 222.00
---	---------	-----------

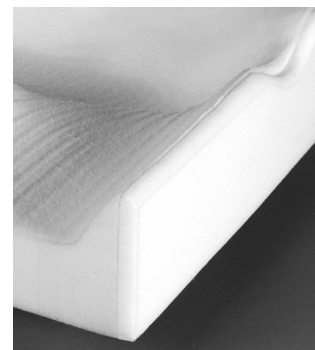

The Lateral Thigh Support Reinforcement option removes 1/2" of cushion foam from each lateral thigh support. Reinforcement material replaces the foam that was removed, without increasing the overall width of the cushion.

# Ride® Custom AccuSoft® Cushion Order Form

Client First and Last Name \_\_\_\_\_

## 8. Modifications

Item	Part Number	Mfr. Sugg. Retail Price*
<input type="checkbox"/> Undercut front edge 1"	RCAC-UC1	\$ 79.00
<input type="checkbox"/> Front rigging notches _____ " W x _____ " D x _____ " H	RCAC-WCFR	\$ 91.00

## 9. Covers

Item	Part Number	Mfr. Sugg. Retail Price*
<input type="checkbox"/> For the outer breathable spacer fabric zip cover included with cushion (if selected)		
<input type="checkbox"/> Spandex layer over spacer fabric	RCAC-SP	\$ 86.00
<input type="checkbox"/> Two-layer spacer fabric Soft Fit	RCAC-EM2	\$ 156.00
<input type="checkbox"/> Additional breathable spacer fabric zip cover	RCAC-CBZA _____ (width)	\$ 226.00
<input type="checkbox"/> Spandex layer over spacer fabric	RCAC-SP	\$ 86.00
<input type="checkbox"/> Two-layer spacer fabric Soft Fit	RCAC-EM2	\$ 156.00
<input type="checkbox"/> Additional outer incontinent-resistant cover Note: Only recommended for chronically incontinent clients. Does not replace inner, moisture-resistant cover.	RCAC-ICA	\$ 272.00
<input type="checkbox"/> Additional inner incontinent-resistant cover	RCAC-INICA	\$ 272.00

## 10. Additional Custom AccuSoft Accessories/Items

Item	Part Number	Mfr. Sugg. Retail Price*
<input type="checkbox"/> 1" / 3cm Cushion Orientation Wedge (These are loose wedges. For a built-in wedge, please see pg. 3.)		
<input type="checkbox"/> For 14" / 36cm cushion widths	RCAC-OW-1414	\$ 87.00
<input type="checkbox"/> For 15" / 38cm and 16" / 41cm cushion width	RCAC-OW-1616	\$ 87.00
<input type="checkbox"/> For 17" / 43cm and 18" / 46cm cushion widths	RCAC-OW-1816	\$ 87.00
<input type="checkbox"/> For 19" / 48cm and 20" / 51cm cushion widths	RCAC-OW-2016	\$ 87.00
Wedge to be used: (select one)		
<input type="checkbox"/> Outside cover		
<input type="checkbox"/> Inside cover		
If inside cover, thick edge of the wedge to be placed:		
<input type="checkbox"/> Back of cushion		
<input type="checkbox"/> Front of cushion		
<input type="checkbox"/> Left side of cushion		
<input type="checkbox"/> Right side of cushion		
<input type="checkbox"/> Ride CAM® Wedge Kit**	RCAC-WK	\$ 41.00

## 11. Growth

Item	Part Number	Mfr. Sugg. Retail Price*
<input type="checkbox"/> Growth Kit Provides for one growth adjustment, including one new inner cover, and one new outer cover during two year warranty period. Width and/or length, and/or height only. Changes in pelvic alignment and body shape can not be accommodated through growth adjustment. (This option requires shipping cushion to Ride Designs with RA.)	RCAC-DGK	\$ 279.00

Total: \_\_\_\_\_

Page 7

We offer a 90 day fit and function guarantee and a two year warranty for all our custom products. Details can be found on our website at [www.ridedesigns.com](http://www.ridedesigns.com).

Continue on page 8

\* All prices are in U.S. dollars.

\*\* One size fits all. Trim in field for correct fit.

**Ride® Custom AccuSoft® Cushion Order Form**

**Client First and Last Name** \_\_\_\_\_

**Special Instructions or Comments**

NOTE: May affect price; call to request quote.

\_\_\_\_\_  
\_\_\_\_\_  
\_\_\_\_\_  
\_\_\_\_\_  
\_\_\_\_\_  
\_\_\_\_\_  
\_\_\_\_\_

**Pair the Ride Custom AccuSoft Cushion with a Ride Custom Back Support for optimal seating**

Consider Ride Designs’ lightweight, thin-profile, and adjustable Custom Back support for the widest range of seating needs.

**Breathable**

Ultra-breathable 3D mesh liner material, along with a washable spacer fabric cover, help to keep the sitter dry and comfortable in virtually any climate. (Requires Level 2 Certification).

**Forgiving**

An optional, soft open-cell polyurethane foam insert is available as an alternative to the ultra-breathable mesh liner.

**Protection and comfort**

Supplementary padding and reliefs improve protection and comfort at sensitive areas.

**Easy to clean and adjust**

Removable cover eases cleaning, maintenance, and adjustments.

**Mounting options**

Strong shell provides stability and surfaces for easy mounting of hardware and accessories.

**Growable**

Like the Ride Custom AccuSoft Cushion, the Back can be grown at a fraction of the cost of a new custom system.

More information at [www.ridedesigns.com](http://www.ridedesigns.com)



Ride Custom Back paired with the Ride Custom AccuSoft Cushion.

\* All prices are in U.S. dollars.



**Ride Designs®**  
a branch of Aspen Seating, LLC



toll-free 866.781.1633  
phone 303.781.1633  
fax 303.781.1722

[www.ridedesigns.com](http://www.ridedesigns.com)  
[customerservice@ridedesigns.com](mailto:customerservice@ridedesigns.com)





# Ride® Custom Back with AccuSoft Foam LIner Order Form

Client First and Last Name \_\_\_\_\_

Prices effective January 8, 2024.

## ► Shape capture method

### Using RideWorks® app?

Before scanning, on the clear, outer shape capture bag (using a black permanent marker), draw trim lines and marks to draw the back as it should be manufactured, including:

- Arrow pointing upward, indicating top of back
- Soft relief areas to protect bony prominences
- Depth and height of the lateral trunk supports



**Before transferring client from shape capture bag, please complete the following...**

**PHOTOS** of client in shape capture bag:  Front view  Side view

- Included in RideWorks® client files
- Emailed to customerservice@ridedesigns.com, with client name and provider information
- Attached

Trim lines; establish and mark on clear, outer shape capture bag:

- Back height
- Lateral support depth and height
- Iliac crest height

DID YOU SEND  
**PHOTOS?**




## ► Using client measurements and final product dimensions? (No scan required. Only available with AccuSoft foam liner.)

Please see ordering instructions on page 10. Please skip to page 11 if ordering with a scan of a captured shape.

**Ride® Custom Back Order Form**  
**Client First and Last Name** \_\_\_\_\_

**Ordering with no scan - just client measurements and finished product dimensions.** (Skip to pg 12 if submitting a scan.)

**⚠ Important:** Clients who present with significant postural asymmetries and require substantial support to maintain optimal posture will experience the best outcome with a Ride Custom Back made from a captured shape that is scanned and submitted to Ride.

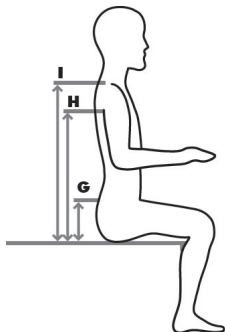


**Step 1 - Client Measurements**


Make sure the following client measurements are provided, either on page 2, or here:

- G. Top of Iliac Crest      L \_\_\_\_\_ "      R \_\_\_\_\_ "
- H. Axilla Height            L \_\_\_\_\_ "      R \_\_\_\_\_ "
- I. Top of Shoulder          L \_\_\_\_\_ "      R \_\_\_\_\_ "

**Step 2 - Desired finished back height \_\_\_\_\_ "**




**Step 3 - Desired finished lateral height from seat to top of lateral. (For full-height lateral pads, this number should equal "tall" lateral pad measurement in step 4. )**




- 3a. Client's left side top of lateral \_\_\_\_\_ "
- 3b. Client's right side top of lateral \_\_\_\_\_ "

**Step 4 - Desired finished lateral pad dimensions (Min. 3" tall.) (Maximum lateral depth, 7". If lateral depth greater than 7" is needed, please capture a shape, scan the shape and submit the scan via the RideWorks app.)**



- 4a. Client left lateral pad \_\_\_\_\_ " tall x \_\_\_\_\_ " deep
- 4b. Client right lateral pad \_\_\_\_\_ " tall x \_\_\_\_\_ " deep

**Step 5 - Desired finished outside back width \_\_\_\_\_ "** (Foam liner will result in inside width being approximately 2" narrower than outside width).

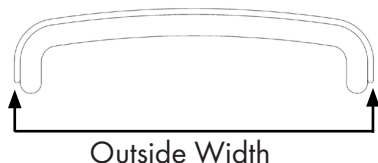

**Ride® Custom Back Order Form**

Client First and Last Name \_\_\_\_\_

**1. Ride Custom Back Type**

Item	Part Number	Mfr. Sugg. Retail Price*
<input type="checkbox"/> <b>Ride Custom Back</b> Medicare HCPCS Code E2617 Custom contoured seat back shell; AccuSoft® foam liner; and choice of removable spacer fabric cover or wipeable, incontinence-proof cover.	RCB200	\$ 2299.00


Minimum back height requirements for headrest accessory use		
Headrest Type	with Single Hardware	with Double Hardware
None	7"/0.178m	12"/0.330m
Universal Headrest Mounting Plate	11.5"/0.292m	18"/0.457m
Integrated Headrest/Accessories Mount	9.5"/0.241m	15.5"/0.394m

NOTE: Measure back height from top trimline to bottom trimline.

**2. Ride Custom Back Size**

Item	Part Number	Mfr. Sugg. Retail Price*
------	-------------	--------------------------

Find the widest spot on client's body in between axilla and trochanters and provide the measurement \_\_\_\_\_"

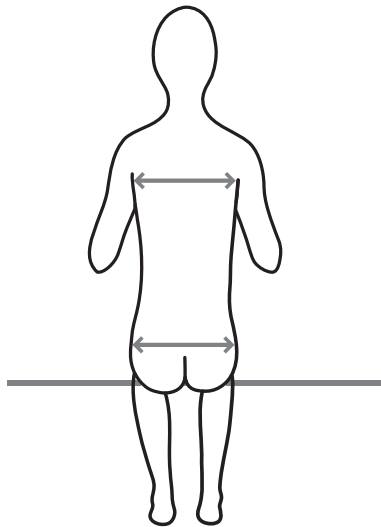

- Widest spot is < 20" RCB2-200R \$ 0.00
- Widest spot is 21" - 24" RCB2-200W \$ 365.00

Pricing for widths greater than 24" will be individually determined and quoted.

\* All prices are in U.S. dollars.

### 3. Ride Custom Back Hardware and Mounting

Item	Part Number	Mfr. Sugg. Retail Price*
------	-------------	--------------------------

#### Ride FlexLoc® Hardware

NOTE: Sections a, b, and c **MUST** have a selection.

##### a. Select Quantity and Size:

NOTE: Order the hardware size that matches the distance between mounting locations, not necessarily the wheelchair width. Mounting FlexLoc to a Permobil or Quantum chair requires small FlexLoc hardware with FlexLoc adapter plates from Ride Designs and a Direct Backrest Frame from Permobil or aftermarket back interface from Quantum.

\*WARNING! Two (2) sets of FlexLoc hardware are required if the client presents with any of the following:

- Weight exceeds 250 pounds
- Overall back height measurement (as measured to trim lines on cast) is greater than or equal to 28"
- Severe extensor tone, spasticity, etc.

Single Set of Hardware

Double Set of Hardware

Small, mounting distance 10 - 14"

Medium, mounting distance 15 - 18"

Large, mounting distance 19 - 21"

X-Large, mounting distance 22 - 24"

Omit hardware

	Part Number	MSRP per set
	RCB2-FL-MS	\$ 590.00
	RCB2-FL-MM	\$ 590.00
	RCB2-FL-ML	\$ 590.00
	RCB2-FL-MX	\$ 590.00
	RCB2-200R-0	\$ 0.00

##### b. Select Mounting:

Clamp Mount for round back canes

Additional Mounting Clamps (pair)

NOTE: If ordering Double FlexLoc mounting hardware, two sets of mounting clamps are included.

Quickie Sedeo Pro Interface Bracket  
 Mounts RCB200 to Quickie Sedeo Pro Power Seating System.

- Not compatible with Quickie Sedeo Pro Advanced seating system.
- Not compatible with tilt-only Sedeo Pro seating system. *Call for mounting options for tilt-only.*
- Available as a single-mount option. *Call for options if double hardware is needed on a Sedeo Pro seating system.*
- Order small FlexLoc hardware for use with this option.
- This option replaces cane clamps.

FlexLoc Adapter Plate  
 For mounting to wheelchairs without round back canes, e.g. Permobil 3G, Invacare Tilt and Recline, or general surface mounting to existing back pans. This option replaces cane clamps.

	RCB2-FL-MCI	Standard
	RCB2-FL-MC	\$ 238.00
	RCB2-QSIB	\$ 205.00

##### c. Select Attachment:

Fixed, non-removeable


Quick Release Option

	RCB2-FL-FMI	Standard
	RCB2-FL-QR	\$ 97.00

NOTE: The Ride FlexLoc Mount can be interfaced with most any wheelchair configuration. Contact Ride Designs for a solution to your mounting challenge.



Ride FlexLoc Hardware on RCB200

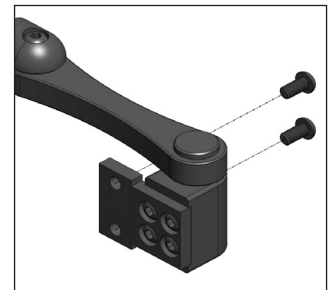

Adapter Plate



Quick Release Option

# Ride® Custom Back Order Form

Client First and Last Name \_\_\_\_\_

## 4. Foam Liner

Item	Part Number	Mfr. Sugg. Retail Price*
------	-------------	--------------------------

Please note: 3D mesh liner is only available to Level 2 Ride Certified Practitioners

- AccuSoft foam liner (increases each lateral support thickness by 1/2" and may result in compromise of postural correction)
  - For AccuSoft foam liner option, select one cover:
    - Spacer fabric cover RCB2-SFC \$ 0.00
    - Wipeable, incontinence-proof cover RCB2-IC \$ 0.00 (Available for AccuSoft foam liner option only)



AccuSoft foam liner

## 5. Supplementary Padding, Reliefs, Dimensions

Item	Part Number	Mfr. Sugg. Retail Price*
------	-------------	--------------------------

- Enhanced relief RCB2-ERFP \$ 354.00
 

Typically used for improved protection and comfort at specific skeletal prominences such as rib humps and spinous processes.

– Draw desired location(s) and shape of relief on clear, outer shape capture bag, or on cast if not using RideWorks.

### Axillary support pad

Typically used for distribution of corrective forces near the axilla on concave side of scoliosis.

- Left RCB2-ASP-L \$ 207.00
- Right RCB2-ASP-R \$ 207.00

### Extended depth lateral thoracic support

- Extend LEFT lateral thoracic support \_\_\_\_\_" forward of reference line. RCB2-EDLTS-L \$ 344.00
  - Extend RIGHT lateral thoracic support \_\_\_\_\_" forward of reference line. RCB2-EDLTS-R \$ 344.00
- Mark reference line(s) on clear, outer shape capture bag, or on cast if not using RideWorks.

### Extended height lateral thoracic support

- Increase LEFT lateral thoracic support \_\_\_\_\_" above reference line. RCB2-EHLTS-L \$ 226.00
- Increase RIGHT lateral thoracic support \_\_\_\_\_" above reference line. RCB2-EHLTS-R \$ 226.00

### Extended back height

- Extend back height \_\_\_\_\_" above reference line. RCB2-EBH \$ 344.00
- Mark reference line(s) on clear, outer shape capture bag, or on cast if not using RideWorks.

- Reinforced lateral thoracic supports RCB2-RLTS \$ 450.00
- Note: No longer required for lateral supports more than 6" deep. It is not possible to adjust lateral width on the RCB200 by bending the lateral reinforcement. Modifications to lateral support width must be made by heating the RCB200 shell.

- Vertical back reinforcement RCB2-RBS \$ 332.00

**PHOTOS??**  
JUST CHECKING.

\* All prices are in U.S. dollars.

## Ride® Custom Back Order Form

Client First and Last Name \_\_\_\_\_

### 5. Accessories

Item	Part Number	Mfr. Sugg. Retail Price*
<input type="checkbox"/> Universal headrest mounting plate, installed Note: Will be installed midline, top of back, unless otherwise marked on clear, outer shape capture bag, or on cast if not using RideWorks.	RCB2-UHMP	\$ 191.00
<input type="checkbox"/> Integrated headrest/accessories mount Note: May be mounted to FlexLoc vertical track if back height is not sufficient for an integrated mount.	RCB2-AM	\$ 284.00
<input type="checkbox"/> Shoulder harness guides, pair, loose	RCB2-SHG	\$ 115.00
<input type="checkbox"/> Shoulder harness guides, pair, installed Note: Mark location on clear, outer shape capture bag, or on cast if not using RideWorks.	RCB2-SHGI	\$ 196.00




Universal Headrest Mounting Plate.

#### Privacy flap

Covers gap between cushion and back support.

##### Size

<input type="checkbox"/> Small — fits wheelchair widths less than 14"	RCB2-PFS	\$ 155.00
<input type="checkbox"/> Medium — fits wheelchair widths 15 - 17"	RCB2-PFM	\$ 155.00
<input type="checkbox"/> Large — fits wheelchair widths 18" and larger	RCB2-PFL	\$ 155.00

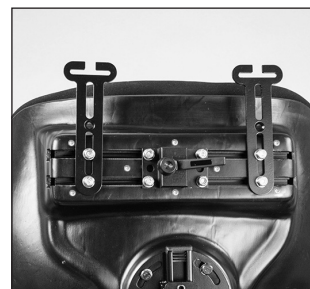

Integrated Headrest/Accessories Mount with Shoulder Harness Guides and headrest mount installed.

#### Abdominal support panel

Instructions:

1. Before removing client from back shape capture bag, mark height of each ASIS on clear, outer bag.
2. Measure up from this mark to establish desired height of abdominal panel needed.
3. Ride Designs will install the abdominal panel for you to meet these specifications.

##### Size

<input type="checkbox"/> Small — height 4" (two straps) Measurement around abdomen _____"	RCB2-AP-4	\$ 408.00
<input type="checkbox"/> Medium — height 6" (three straps) Measurement around abdomen _____"	RCB2-AP-6	\$ 408.00
<input type="checkbox"/> Large — height 8" (three straps) Measurement around abdomen _____"	RCB2-AP-8	\$ 408.00



Privacy flap covers the space between the cushion and back support.

### 6. Covers

Item	Part Number	Mfr. Sugg. Retail Price*
<input type="checkbox"/> Additional breathable cover	RCB2-SFCA	\$ 384.00
<input type="checkbox"/> Additional wipeable, incontinence-proof cover	RCB2-ICA	\$ 384.00



Abdominal Support Panel.

### 7. Growth

Item	Part Number	Mfr. Sugg. Retail Price*
<input type="checkbox"/> Growth Kit Provides for one growth adjustment, including a new cover, during two year warranty period. Width and/or height only. Changes in spinal alignment and body shape can not be accommodated through growth adjustment.	RCB2-DGK	\$ 512.00

Total: \_\_\_\_\_

